

Fig. 1 (Conventional)

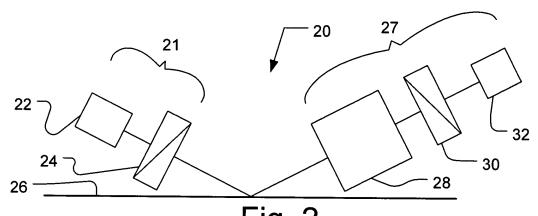


Fig. 2 (Conventional)

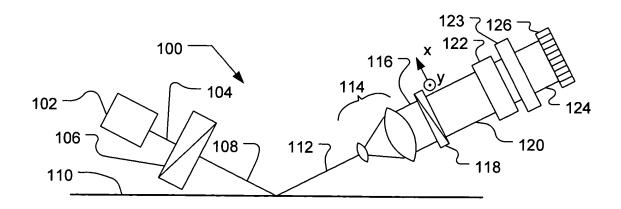


Fig. 3

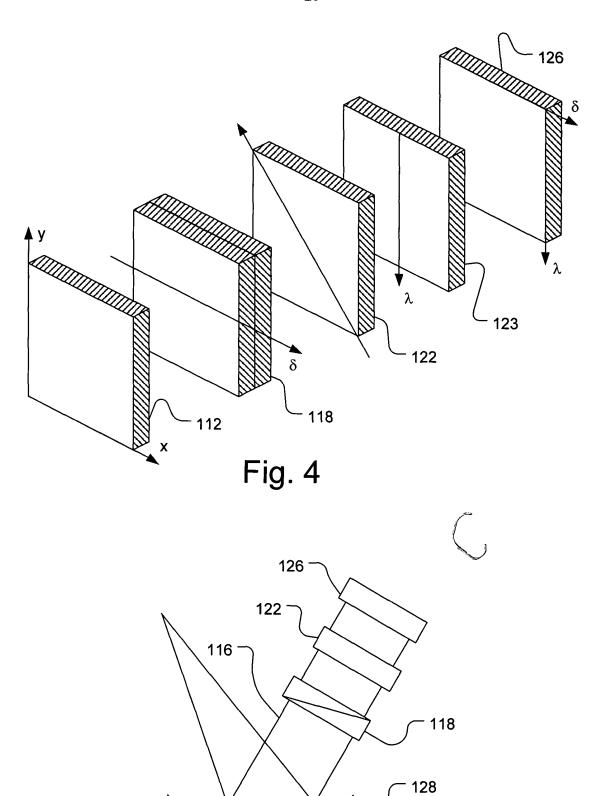


Fig. 5

Title: Reference Calibration of Metrology Instrument First Inventor: Chunsheng Huang Docket Number: NAN065 US 3/9

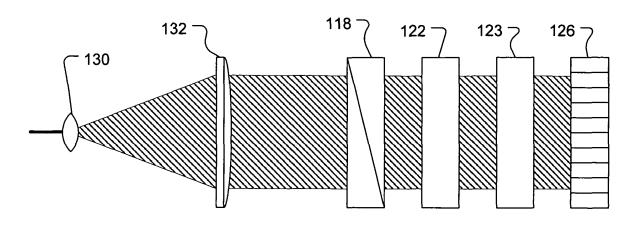


Fig. 6A

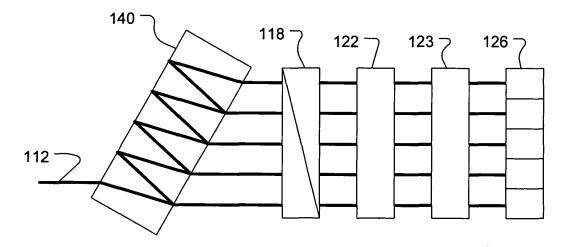


Fig. 6B

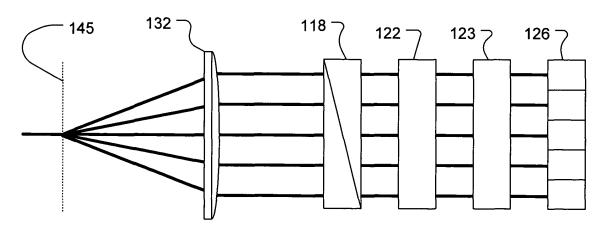


Fig. 6C

Title: Reference Calibration of Metrology Instrument First Inventor: Chunsheng Huang Docket Number: NAN065 US 4/9




Fig. 7A




Fig. 7B




Fig. 7C

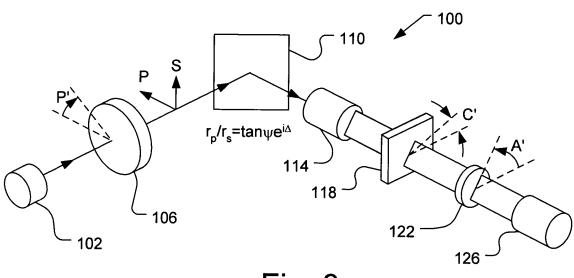


Fig. 8



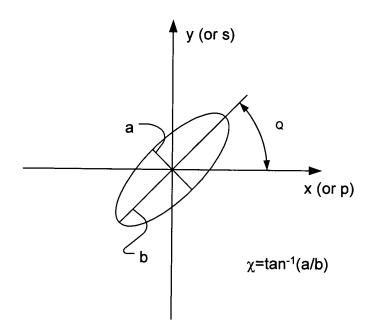


Fig. 9

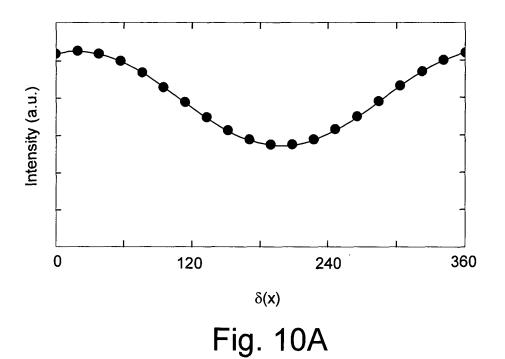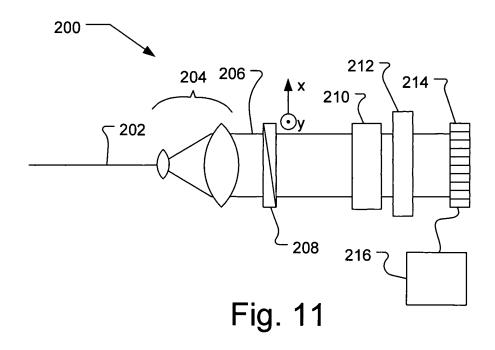

 $\begin{array}{c} \text{Tuteusity (a.u.)} \\ \text{O} \\ \text{120} \\ \text{240} \\ \text{360} \\ \end{array}$

Fig. 10B



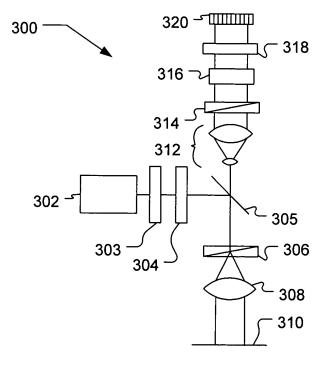


Fig. 12

Title: Reference Calibration of Metrology Instrument First Inventor: Chunsheng Huang Docket Number: NAN065 US 8/9

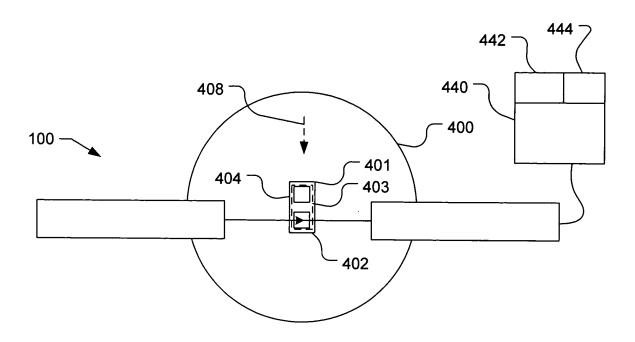


Fig. 13

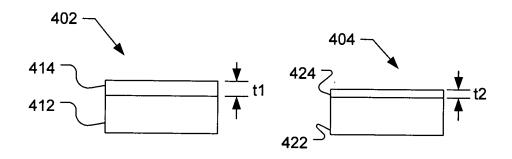


Fig. 14A

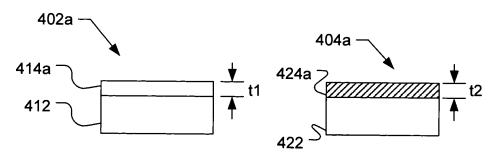


Fig. 14B

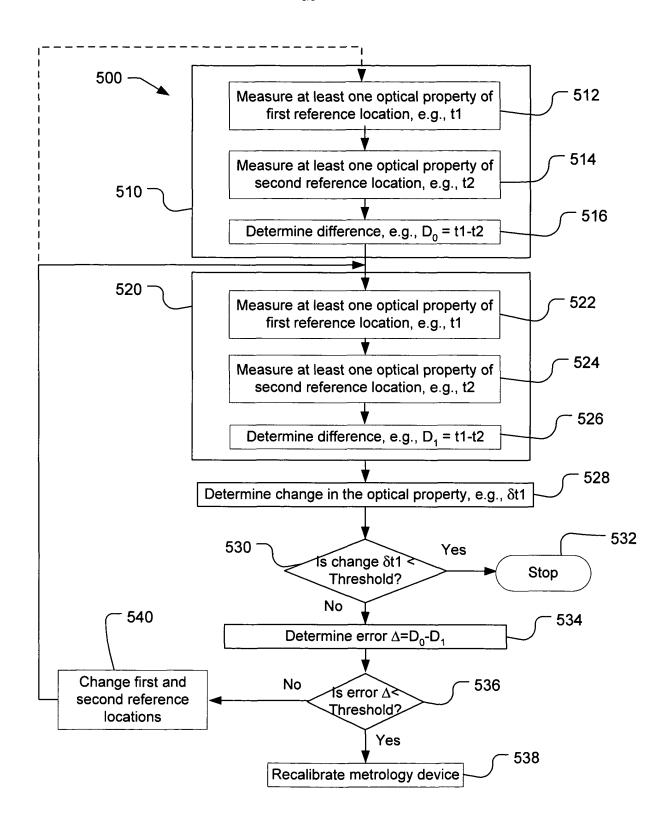


Fig. 15